

## 产品分析证书 Certificate of Analysis

中文名称: Alpha-乳香酸

English Name: Alpha-Boswellic acid

别名 (Alias): 3alpha-Hydroxy-12-oleanen-24-oic acid

产品编码 (Cat. No.): BP0153


CAS Number: 471-66-9

分子式 (M. F.): C<sub>30</sub>H<sub>48</sub>O<sub>3</sub>

分子量 (M. W.): 456.711

批号 (Batch No.): PRF8052701

报告日期 (Report date): 2017-05-27

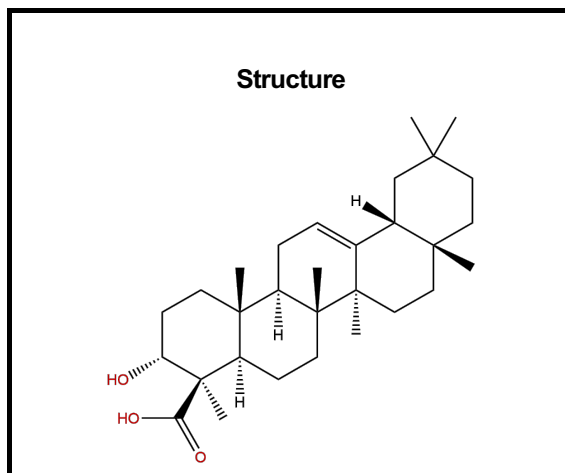

**检验结果 (Analytical result):**

检验项目 (Test Item)	检验指标 (Specifications)	检验结果 (Results)
外观 Appearance	Off-white powder	Off-white powder
干燥失重 Loss on drying	<3.0%	0.94%
纯度 Purity (HPLC-DAD, 205nm)*	≥98.0%	99.25%
质谱 Mass	456.7±1	Conforms
核磁 NMR	Comply with the structure	Conforms

\* 色谱图见附件 (Please find HPLC chromatography attached.)

检测方法 (Test Method): Column: Agilent 5TC-C18, 4.6\*150mm; Column temperature: 30°C; Detection Mode: UV205nm; Flow Rate: 1.0ml/min; Sample dissolution: Methanol; Mobile Phase: A, 0.1% phosphoric acid in water B, Acetonitrile; Gradient elution: B, 80%-95%, 15min.

贮存条件 (Storage): -2~8°C, protected from light, keep package airtight when not in use.

复测期 (Retest date): two years (2019-05-26) under conditions list above.

QC: Zhang Ling  
Date: 2017-05-27

QA: Wu Qi  
Date: 2017-05-27

备注 (Remarks): The sample solutions should be prepared and used immediately. It is the best preparing the solutions immediately before use. If the solutions have to be made up in advance, it should be made as aliquots in tightly sealed vials at less than -20°C. Generally, these might be useable for up to two weeks.  
In case of quality issue, please contact us within 15 days after receipt of the product.


Tel: +86-28-82633397 Fax: +86-28-82633165

http://www.phytopurify.com Email: sales@biopurify.com biopurify@gmail.com

**SAMPLE INFORMATION**

Sample Name:	Alpha-Boswellic acid PRF8052701	Acquired By:	System
Sample Type:	Standard	Sample Set Name:	
Vial:	72	Acq. Method Set:	Alpha-Boswellic acid
Injection #:	1	Processing Method:	Samples
Injection Volume:	10.00 ul	Channel Name:	205.0nm
Run Time:	25.0 Minutes	Proc. Chnl. Descr.:	PDA 205.0 nm
Date Acquired:	2017-5-27 10:39:03 CST		
Date Processed:	2017-5-27 11:06:21 CST		

**Auto-Scaled Chromatogram**

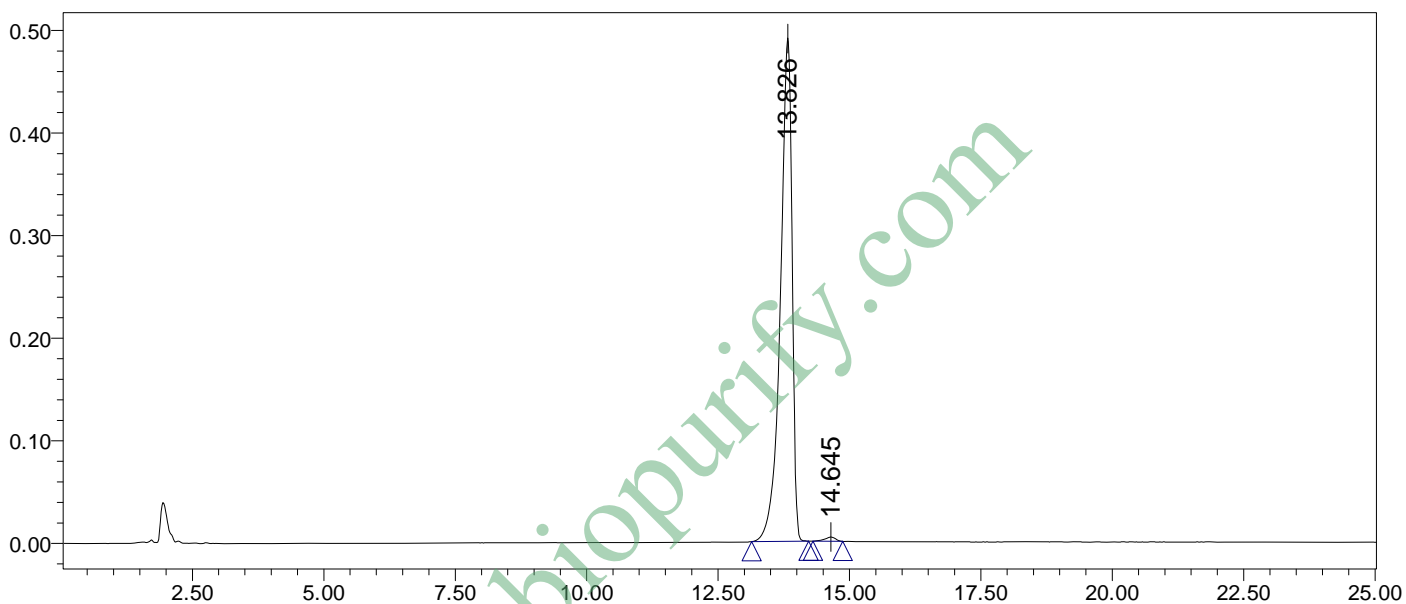

**Peak Results**

	RT	Area	% Area	USP Plate Count	USP Resolution
1	13.826	7536789	99.25	19784.87	
2	14.645	57035	0.75	24686.61	2.09